

FIG. 2

0994407-11504
FIG. 2

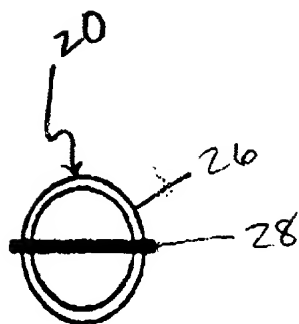



FIG. 3

Docket No. PPC-812



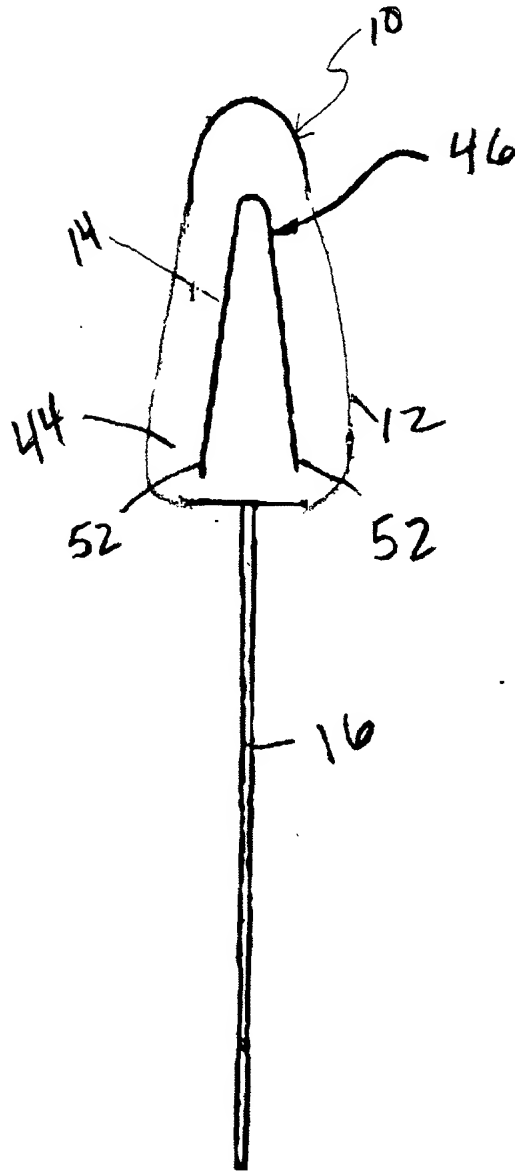


FIG. 5

FO97T 2047660

09091407 111601

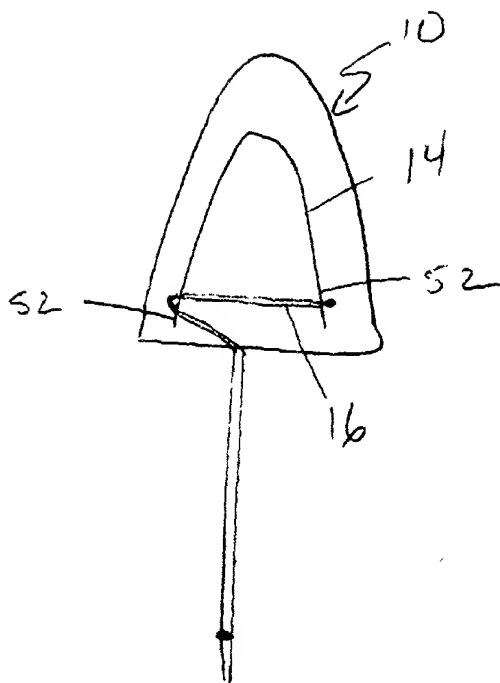


Fig. 5a

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

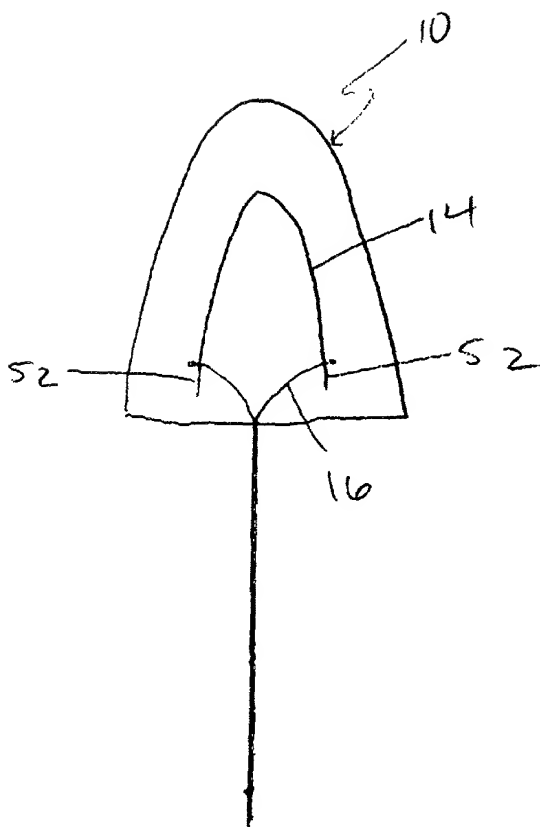


FIG. 5b

0903407 11601

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

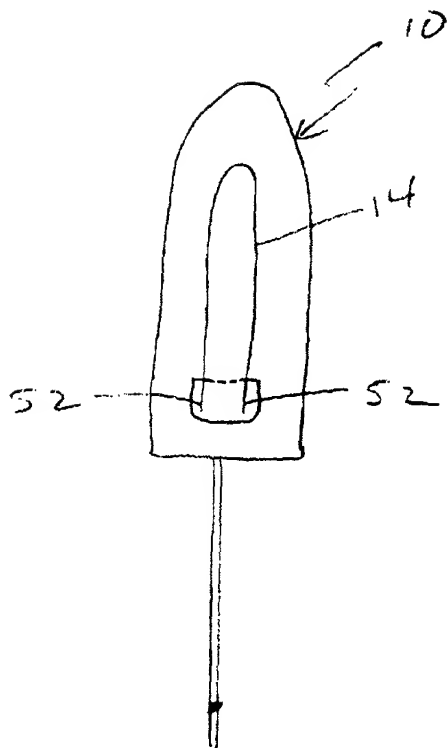


FIG. 5 C

FIG. 5 C

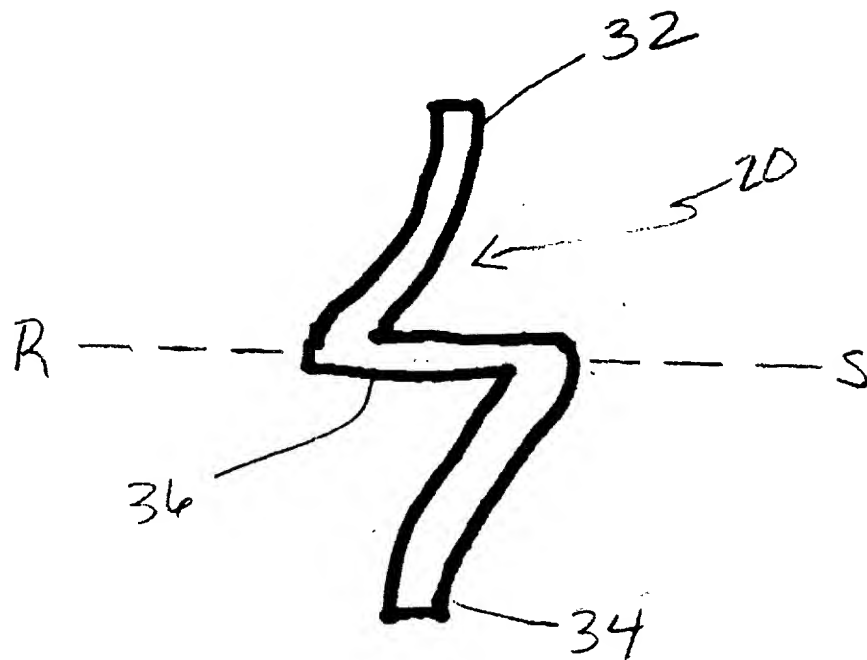


FIG. 6

FIG. 6

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

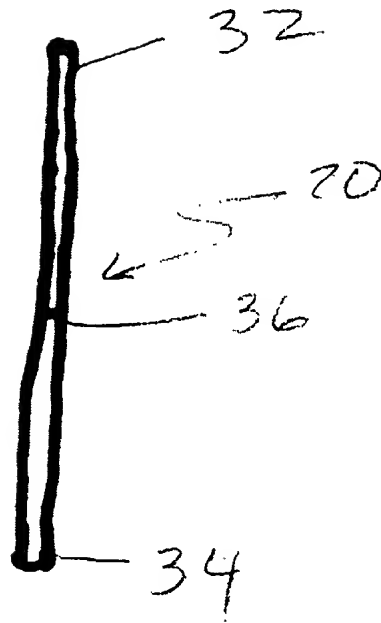


FIG. 7

09991403-11601


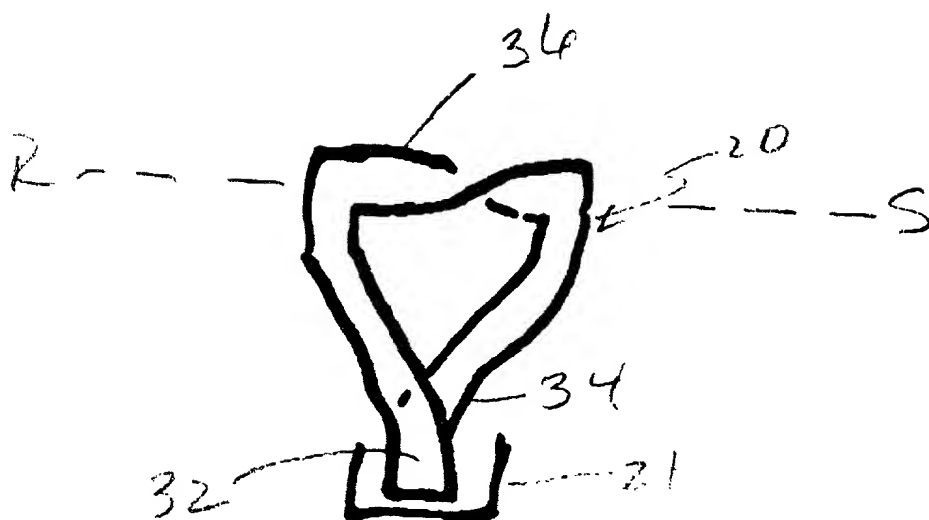


Fig. 8

09931407, 111601
109777/2046660

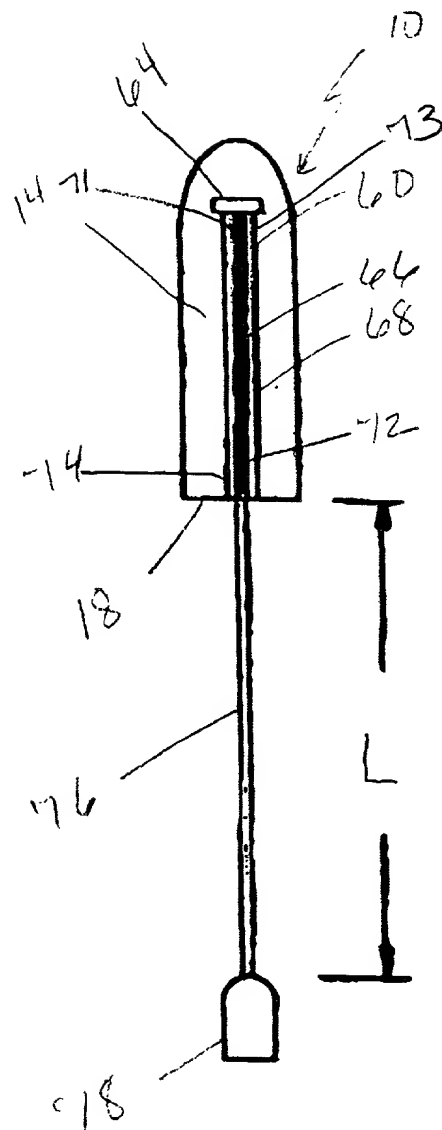

F16.9

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

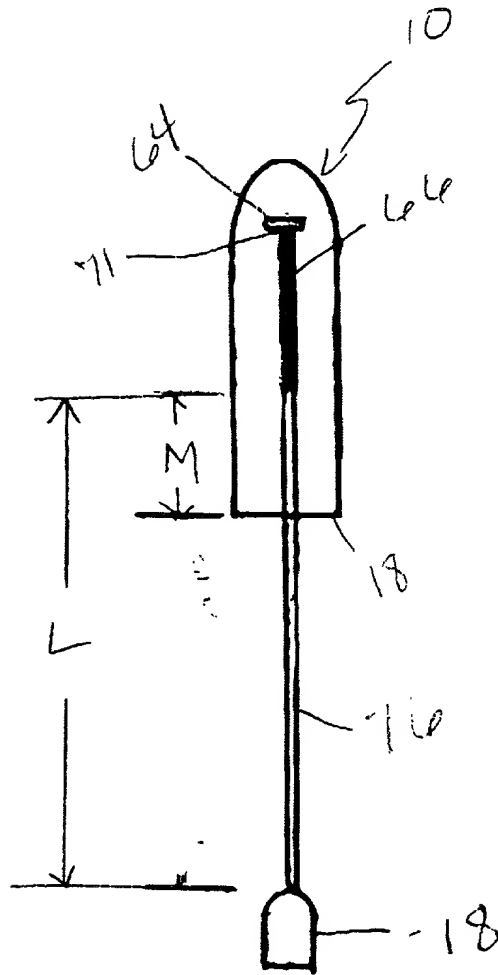


Fig. 16. 10

09991407-111601

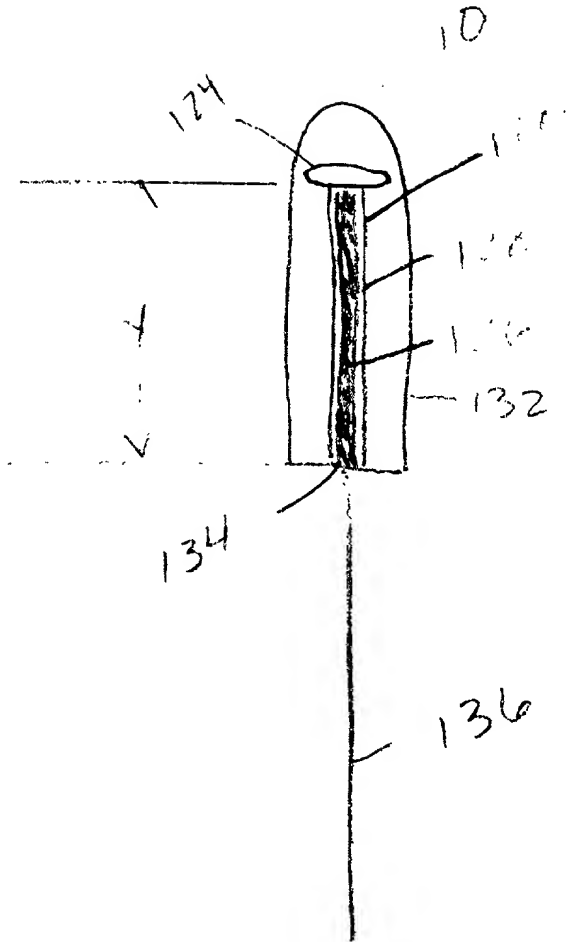



Fig. 11

FIG. 11

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

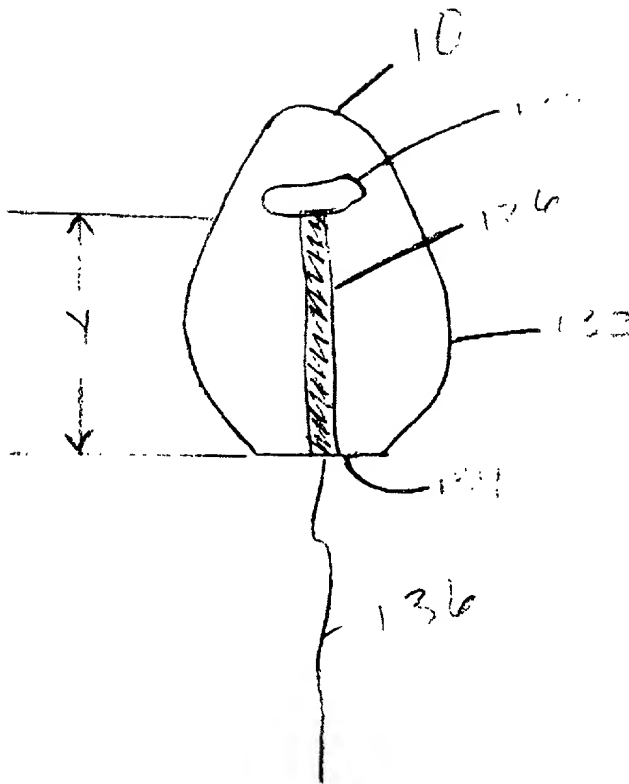

116.12

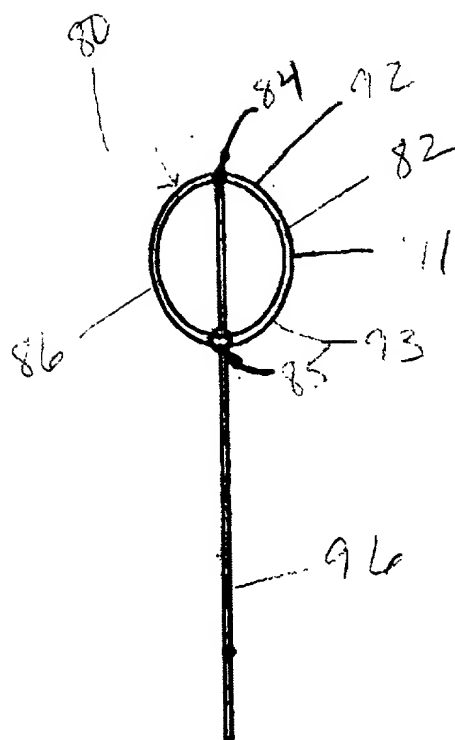


FIG. 13

0991467, 111601

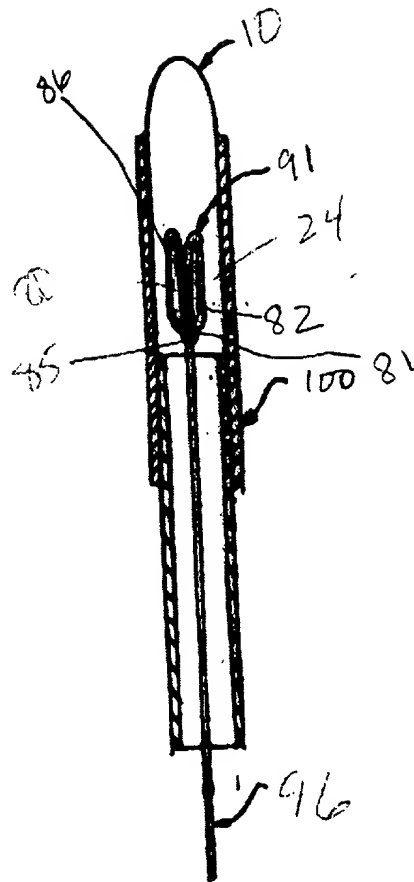


FIG. 14

FIG. 14

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

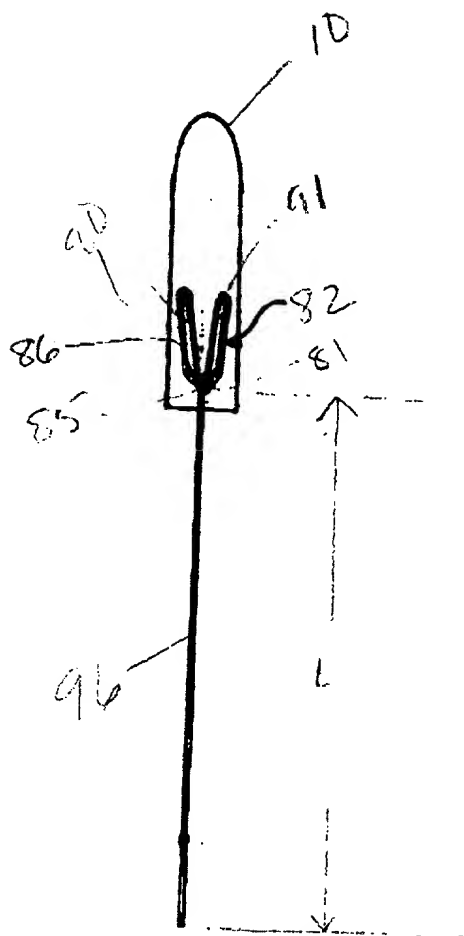


FIG. 15

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

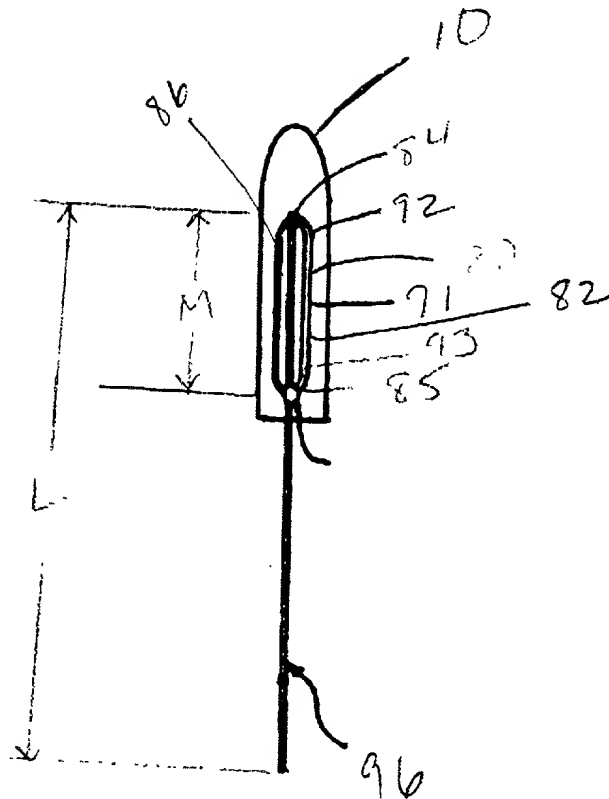


FIG. 16

09991407.111601

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

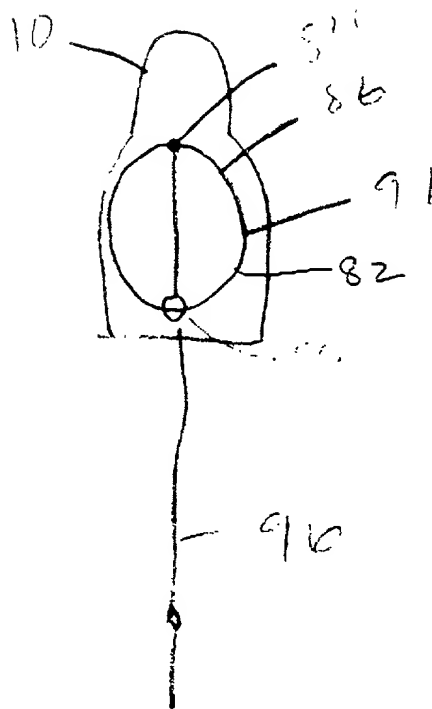


Fig. 17

05991407, 111501